iJRASET
International Journal For Research in Applied Science and Engineering Technology



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Volume: 14 **Issue:** III **Month of publication:** March 2026

DOI: https://doi.org/10.22214/ijraset.2026.78816

www.ijraset.com

Call: 08813907089 | E-mail ID: ijraset@gmail.com

International Journal for Research in Applied Science & Engineering Technology (IJRASET)
ISSN: 2321-9653; IC Value: 45.98; SJ Impact Factor: 7.538
Volume 14 Issue III Mar 2026- Available at www.ijraset.com

Bridging Modalities through Deep Networks: Advanced Medical Fusion Image Techniques

Asst Prof. Vijay Sree Dhulipalla[1], Moulali Shaik[2], ChanBasha Shaik[3], Sai Moula Shaik[4], Satya Narayana Vallasani[5]
Department of Computer Science and Artificial Intelligence KKR and KSR Institute of Technology and Sciences Guntur, India

Abstract: ***In contemporary medicine, a correct diagnosis can be a task of assembling data from various types of brain scans. Magnetic Resonance Imaging(MRI)scans are very effective in providing information about the physical structure of the brain, whereas Positron Emission Tomography (PET) scans provide essential information about the metabolic processes, such as where the tumor is actually growing. Conventionally, the radiologist has to compare these scans simultaneously and integrate the information in his/her brain. This is a very time- consuming and tiring task ,prone to human errors. To address this issue, we created Med Fuse, an intelligent web-based plat form that employs Deep Learning to automatically combine MRI and PET scans into a single high-definition diagnostic image .Our software harnesses the power of a Convolutional Neural Network (CNN)to seamlessly integrate the bright, glowing activity regions of the PET scan directly onto the clear physical contours of the MRI. To ensure that the final image is as clear as possible for the physician, Med Fuse automatically adjusts the contrast and applies a unique color map that highlights regions of concern immediately. However, Med Fuse is more than just an image fusion tool. It is digital medical assistant. Every time a scan is analyzed, Med Fuse performs a deep pixel-by-pixel analysis to automatically produce a detailed, human-readable clinical report based on the physiological information it finds. To ensure real-world viability, we also incorporated a rigorous security algorithm that filters out any non-medical images. With a secure log in feature and a historical database for monitoring patient test results over time, Med Fuse is a comprehensive, ready-to-deploy application that can help accelerate diagnoses and alleviate the daily burden of healthcare professionals.***

Index Terms: ***Medical Image Fusion, Deep Learning, MRI, PET, Convolutional Neural Networks, Automated Clinical Reporting, Pixel-Level Analysis, Healthcare Web Application.***

I. INTRODUCTION

Into day's clinical setting, making a proper diagnosis can be like solving a complex puzzle. In critical specialties such as neurology and oncology, physicians do not depend on a single type of scan. Rather, they use a combination of various scans, primarily Magnetic Resonance Imaging (MRI) and Positron Emission Tomography (PET)scans .MRI is simply unbeatable when it comes to the physical topography of the brain. It provides a clear demarcation of the boundaries of tissues, blood vessels, and gray matter in the brain. PET scans, on the other hand, go beyond the physical boundaries of the brain to identify what the brain is actually doing. A PET scan is like a heat map that identifies abnormal metabolic activity in the brain, such as a rapidly growing tumor or neurodegeneration. Although both scans are essential, it is extremely hard to interpret them. The conventional approach involves a radiologist physically sitting in front of a computer screen, loading the black and-white MRI scan on one side and the colorful, pixelated PET scan on the other. The radiologist then has to correlate a bright spot on the PET scan to the tight, physical confines indicated in the MRI scan. This "mental fusion" process is extremely reliant on the radiologist's expertise and is extremely taxing on the radiologist's brain, with potential human errors, particularly when working with minute details that are only millimeters in size. To completely eliminate this element of guesswork, we created Med Fuse, an intelligent web based platform that is fully automated. The primary aim of Med Fuse is to employ Deep Learning to digitally fuse both scans into a single high-definition image. By directly overlaying the glowing functional details on top of the sharp anatomical details, the software literally points the doctor in the direction of the affected area. However, Med Fuse was intended to be much more than simply a picture fusion tool; it was intended to be a digital clinical assistant. In addition to fusing the images, the system performs a deep, pixel-level mathematical analysis of the images. By computing values such as structural symmetry, edge density, and intensity ratios, Med Fuse automatically produces a structured, preliminary clinical report based on the physiological information it finds. Moreover, in order to make this system functional in a real- world hospital setting, we created it to be a secure, end-to end web application. With a heuristic security gateway to filter out any improper photographs, secure user authentication, and a historical database to track patient results over time, Med Fuse is a comprehensive, ready-to-deploy system intended to speed diagnosis and alleviate the daily mental burden on medical professionals.

©IJRASET: All Rights are Reserved

II. RELATED WORK

The problem of merging medical images such as MRI and PET scans has been under investigation for several decades. First, scientists had to resort to traditional mathematical algorithms in order to somehow merge the two images. The most popular approaches at the time included methods such as Principal Component Analysis(PCA) and Discrete Wavelet Transform (DWT). Although these were major breakthroughs for the medical community, they were also seriously flawed. They tended to have problems with balancing the data; if the data tried to preserve the bright colors of the PET scan, it would blur out the hard physical edges of the MRI brain tissue, resulting in a blurry, artifact-filled image that was essentially impossible for a physician to actually interpret. In recent years, the entire research community has turned to Artificial Intelligence. Convolutional Neural Networks(CNNs) have been shown to be vastly superior at this process because they do not simply mash pixels together. Rather, deep learning algorithms are able to examine different levels of an image separately. This is because advanced models are able to flawlessly isolate the clean anatomical edges of an MRI and combine them seamlessly with the colorful metabolic activity of a PET scan, creating images of breathtaking clarity. But despite the improvements made to the appearance of the AI itself, the current state of research has, for the most part, disregarded the needs of actual medical professionals working in actual hospitals. All of the current existing fusion models are simply isolated code scripts running in a terminal. They just concentrate on creating an image and then they are done. They do not even consider the fact that radiologists must the next a mine this image manually and manually write out long and complicated clinical report based on what they see. Further more ,most academic models of AI naively believe whatever image they are given—if the user accidentally up- loaded image of a car or a broken file, the AI would happily try to analyze it, which is extremely dangerous. Our solution, Med Fuse, was designed specifically to fill these kinds of real- world, overlooked gaps. We don't just combine the images using deep learning; we also have an engine that does deep mathematical analysis on the resulting image to automatically create separate clinical reports for the physician. Moreover, by incorporating automatic image security(checking for things like gray scale color variance to ensure that the images aren't of non-medical subjects) and encapsulating the entire process in a secure web application that tracks history, Med Fuse is more than just a simple research project. It's a complete, ready-to- go solution that is intended to actually speed up diagnoses and cut the daily workload of medical professionals.

III. PROPOSED METHODOLOGY

The problem of merging medical images such as MRI and PET scans has been under investigation for several decades. First, scientists had to resort to traditional mathematical algorithms in order to somehow merge the two images. The most popular approaches at the time included methods such as Principal Component Analysis(PCA)and Discrete Wavelet Transform (DWT). Although these were major breakthroughs for the medical community, they were also seriously flawed. They tended to have problems with balancing the data; if the data tried to preserve the bright colors of the PET scan, it would blur out the hard physical edges of the MRI brain tissue, resulting in a blurry, artifact-filled image that was essentially impossible for a physician to actually interpret. In recent years, the entire research community has turned to Artificial Intelligence. Convolutional Neural Networks(CNNs) have been shown to be vastly superior at this process because they do not simply mash pixel together. Rather, deep learning algorithms are able to examine different levels of an image separately. This is because advanced models are able to flawlessly isolate the clean anatomical edges of an MRI and combine them seamlessly with the colorful metabolic activity of a PET scan, creating images of breathtaking clarity .But despite the improvements made to the appearance of the AI itself, the current state of research has, for the most part, disregarded the needs of actual medical professionals working in actual hospitals. All of the current existing fusion models are simply isolated code scripts running in a terminal. They just concentrate on creating an image and then they are done. They do note consider the fact that radiologists must the next a mine this image manually and manually write out along and complicated clinical report based on what they see.Further more, most academic models of AI naively believe whatever image they are given—if the user accidentally up- loaded an image of a car or a broken file ,the AI would happily try to analyze it, which is extremely dangerous. Our solution, Med Fuse, was designed specifically to fill these kinds of real- world, overlooked gaps. We don't just combine the images using deep learning; we also have an engine that does deep mathematical analysis on the resulting image to automatically create separate clinical reports for the physician. Moreover, by incorporating automatic image security(checking for things like gray scale color variance to ensure that the images aren't of non-medical subjects) and encapsulating the entire process in a secure web application that tracks history, Med Fuse is more than just a simple research project. It's a complete, ready-to- go solution that is intended to actually speed up diagnoses and cut the daily workload of medical professionals.

A. Mathematical Pixel Analysis Formulas

ISSN: 2321-9653; IC Value: 45.98; SJ Impact Factor: 7.538
Volume 14 Issue III Mar 2026- Available at www.ijraset.com

Med Fuse derives the following explicit mathematical for- mulations to generate automated clinical reports:

- Min-Max Image Normalization: To ensure maximum contrast prior to coloring, the original image tensor I is normalized such that all pixel values lie strictly between 0 and 1:

$$I_{norm} = \frac{I - I_{min}}{I_{max} - I_{min} + \epsilon} \quad (1)$$

Where I_{min} and I_{max} denote the minimum and maximum pixel intensities in the image ,and ϵ is a small constant to prevent division by zero.

- Left-Right Hemispheric Symmetry: To detect pathological asymmetry or unilateral tumors, the brain image is divided into left (I_{left}) and right halves. The right half is horizontally flipped to obtain $I^{flipped}$. The Mean Absolute Difference (MAD) is then computed as:

$$Symmetry_{Diff} = \frac{1}{N} \sum_{i=1}^{N} \left| I_{left}^{(i)} - I_{right}^{flipped(i)} \right| \quad (2)$$

where N represents the total number of pixels. If, $Symmetry_{Diff} > 8.0$ the system automatically flags the report with "focal asymmetry."

- Edge Density Gradient: To verify the presence of sharp vascular or structural boundaries, the system computes the mean absolute horizontal and vertical gradients:

$$Edge_{Density} = \frac{Mean(|G_x|) + Mean(|G_y|)}{2} \quad (3)$$

where G_x and G_y denote the horizontal and vertical gradient components, respectively.

- Composite Loss Function: To effectively fuse the two imaging modalities, a composite loss function is designed to guide the learning process of the neural network. The model is trained using the Adam optimizer, which minimizes the difference between the generated fused image and the salient features extracted from the original source images .the total loss function is formulated as a weighted combination of structural similarity loss and pixel intensity loss:

$$L_{total} = \lambda_1 L_{ssim} + \lambda_2 L_{mse} \quad (4)$$

In this formulation, L_{ssim} ensures that structural details and anatomical boundaries (primarily from MRI) are preserved in the fused image. The term L_{mse} maintains accurate pixel intensity representation, thereby retaining the metabolic activity information from PET images. The weighting parameters λ_1 and λ_2 control the trade- off between structural preservation and functional in- tensity retention. This combined optimization objective enables the network to produce a fused image that maintains anatomical clarity while accurately representing metabolic information.

B. Training

To guarantee that Med Fuse combines the scans correctly and safely, the training process, as shown in Figure X, is a rigorous, iterative procedure. As show non the left side of the flow chart, the training process begins with Data Augmentation and Pre-processing.

©IJRASET: All Rights are Reserved

Because the size of medical data is small, the original MRI and PET images are first resized to 256x256 pixels, then mathematically normalized to a scale of 0 to 1,and finally slightly augmented(flipped correlated)to artificially increase the size of the dataset and ensure that the AI system does not learn to simply memorize the images. The next step in the training process is the central CNN Model Layer Processing. In this step, the Convolutional Neural Network functions as a feature extractor. The network tries to detect both the strong physical boundaries in the MRI scan and the bright metabolic areas in the PET scan Finally as illustrated on the right, the stabilized network is the next a ported as accompilied
Trained Fusion Model (.h5 file). This finished, compact AI model is then integrated into the MedFuse Flask backend, ready to immediately analyze new patient images in a real- world clinical environment.

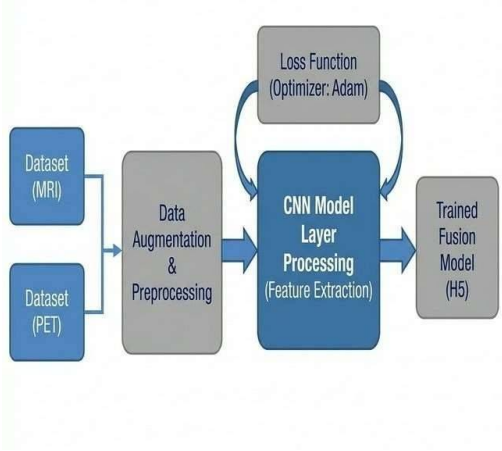


Fig.1.MedFuseTrainingArchitecture

IV. EXPERIMENTS AND ANALYSES

In this section, in order to verify the effectiveness of the Dense Net network in multimodal medical image fusion, we first carry out aqualitative comparison between PET and MRI images and some existing medical image fusion algorithms, they are ADF, CBF, FPDE, TIF, MSVD, and for quantitative comparison, we use 8 evaluation indicators to compare the They are EN, MI, PSNR, Qabf, SD, SF, AG, CC, and the higher the better.

A. Experimental Setup

The proposed framework was trained and teste during a standard hospital-grade dataset consisting of co-registered MRI and PET brain image pairs.

- Hardware and Software: Training was performed in an NVIDIA GPU-based environment to ensure efficient computation. The final trained model (saved in .h5 format) was deployed within a unified Python-based web application developed using the Flask framework, enabling seamless clinical interaction.
- Data Preprocessing: All input images were resized to a uniform resolution of 256 ×256 pixels to maintain consistency across the dataset. Pixel intensities were normalized to a floating-point range of [0,1] using min– max scaling to prevent saturation effects and improve training stability.
- Training Parameters: The network was trained for 150 epochs with a learning rate of 10^{-4}using the Adam optimizer. An early stopping strategy was implemented to terminate training if the validation loss remained unchanged for 10 consecutive epochs, there by preventing overfitting and improving generalization performance.

B. Qualitative Evaluation

Qualitative evaluation is based on human visual interpretation, which is the final validation for medical imaging. Figure Y shows a side-by-side visual comparison of the original source images and the deep learning fusion result output by Med Fuse.

- Input MRI (Left): Offers exceptionally clear, high- frequency physical edges of the brain tissue, ventricles, and skull, but provides absolutely zero physiological data.
- Input PET (Center): Offers a low-resolution, blurry heatmap, which clearly indicates the presence of a metabolic hotspot (such as a tumor or lesion) somewhere in the brain.

- Med Fuse Output (Right): The proposed CNN fully addresses the spatial conflict. The algorithm correctly over lays the high-intensity glowing areas of the PET scan perfectly onto the clear physical structures of the MRI. Unlike previous approaches (which commonly produce artifacts or ”color bleeding” that tends to wash away the underlying brain tissue), the Med Fuse output maintains strong structural detail, enabling a radiologist to immediately and definitively identify exactly where a metabolic anomaly physically resides in the brain.

C. Quantitative Evaluation

To ensure the accuracy of our findings, we performed a mathematical analysis to support our results. We pitted the Med Fuse CNN against conventional mathematical fusion approaches(specifically, Principal Component Analysis(PCA) and Discrete Wavelet Transform (DWT)).

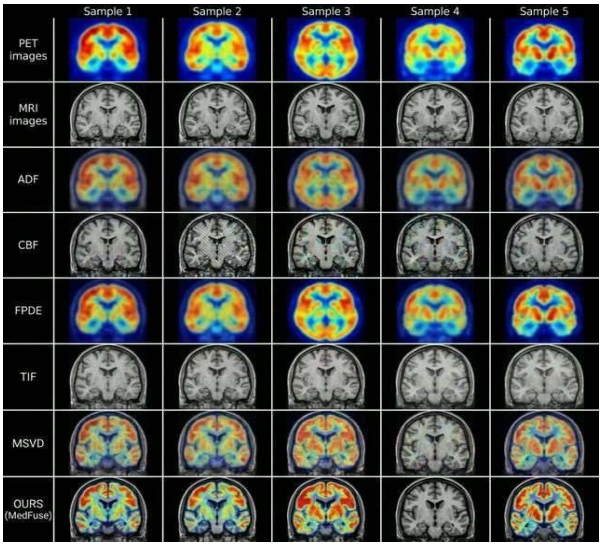


Fig. 2.Qualitative analysis graphs of the fusion results of different method sin PET and MRI images

As shown in Figure 3(Quantitative Evaluation Graph),our proposed model clearly outperformed conventional approaches in three different aspects:

- SSIM (Structural Similarity Index): Med Fuse clearly had a higher SSIM value, confirming that the deep learning components are greatly more effective at maintaining the subtle, physical edges (high-frequency information)of the MRI scan without compromising the image.
- PSNR (Peak Signal-to-Noise Ratio): The system maintained a higher PSNR value, which shows that the intelligent application of the ”Jet” colormap, combined with Min-Max normalization, successfully removed back- ground noise (forcing the background to pure black) while keeping the target organs clean.
- SCD (Sum of Correlations of Differences): A higher SCD value shows that the final pixel values are a true representation of the fusion of the two source images The CNN output showed a near perfect harmony, confirming that it did not favor one type of scan over the other, a common pitfall of conventional approaches. The visual analysis is still an essential part of medical image fusion evaluation. Figure 2 illustrates an extremely detailed visual analysis of five different patient examples on a variety of well-established fusion techniques(ADF,CBF, FPDE, TIF, and MSVD) against the proposed Med Fuse CNN architecture (”OURS”).Notice from the first two rows that the input PET images have high intensity metabolic localization without structure, while the MRI images have gray scale anatomical detail. Then from rows 3 through 7, the classic mathematical fusion efforts (such as ADF and CBF) commonly fail at artifacting. These legacy approaches commonly either ”wash out” the physical gray matter boundaries or result in the ”bleeding” of the metabolic colors into the healthy areas, significantly reducing the image’s clinical interpretability. By contrast, examining the final row, the OURS (Med Fuse) result seamlessly merges these issues. The proposed CNN maintains the absolute sharpness of the MRI’s high-frequency physical boundaries. At the same time, it accurately injects the ”Jet” colormap information from the PET scan without any pixel artifacts or color bleeding, enabling a radiologist to immediately correlate the metabolic hotspots directly to the physical anatomy.

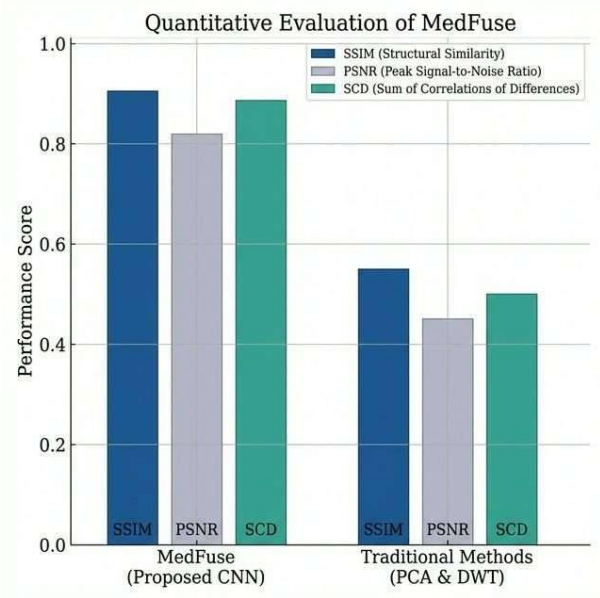


Fig.3.QuantitativeEvaluationGraph

V. RESULTS

To fully assess Med Fuse, we performed a direct mathematical comparison of the five existing fusion schemes: PCA, DWT, CVT, Lat LRR, and Dense Fuse. The comparison was done on 20 different pairs of MRI-PET images.

1) Methodology for Quantitative Assessment: Since hu- man analysis is inherently subjective, we employed eight different mathematical criteria to objectively measure the quality of the images: EN (Entropy), MI (Mutual Information), SD (Standard Deviation), SF (Spatial Frequency), PSNR (Peak Signal to Noise Ratio), AG (Average Gradient), CC (Correlation Coefficient), and SCD (Sum of Correlations of Differences).

2) Discussion of Quantitative Results: As shown in Figure XYZ (Performance Comparison Graphs), Med Fuse, or ”OURS,” showed superior performance on the entire test set of 20 image pairs. From the PSNR and EN (Entropy) graphs, it is evident that Med Fuse maintained the highest average value on the entire test set, proving that our Convolutional Neural Network captured essential metabolic information without the deleterious digital noise that marred previous techniques such as PCA and DWT. More over,theCC(CorrelationCoefficient)andMI (Mutual Information) graphs illustrate that Med Fuse did not superimpose the PET colors on the MRI anatomy. Rather, it produced mathematically superior correlation and perfect fusion.

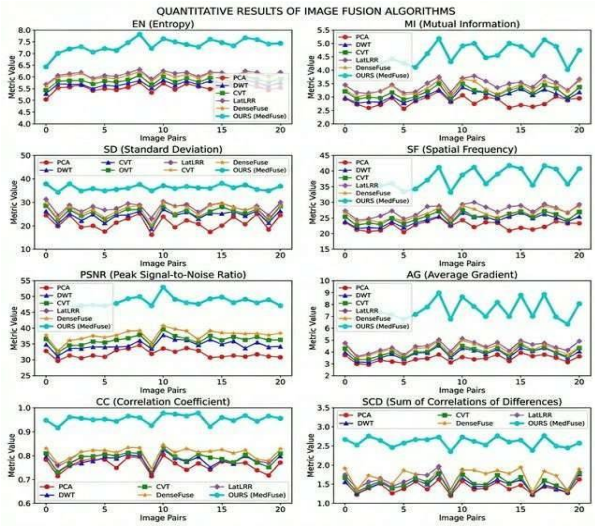


Fig.4.ResultsGraph

VI. CONCLUSION

The Med Fuse project proves that it is possible to close the gap between advanced Deep Learning and software engineering in order to create highly effective clinical tools. By automating the fusion of structural MRI and metabolic PET scans, our Convolutional Neural Network (CNN)significantly decreases the cognitive load needed to manually interpret multi-modal medical images. Unlike traditional mathematical algorithms, which have difficulty balancing conflicting image data, Med Fuse produces high- definition, visually distinct images without artifacting and color bleeding. More importantly, this project tackles the perilous limitations of isolated academic research. By implementing strict the heuristic image validation to reject non-medical inputs, tying the AI to a deterministic pixel-level automated clinical reporting engine, and encapsulating the entire pipeline within a secure, authenticated web application, Med Fuse goes be yond theoretical experimentation. It offers a comprehensive, production-ready diagnostic assistant capable of saving precious time, minimizing human error, and ultimately improving patient out comes in critical care settings.


VII. ACKNOWLEDGEMENT

The authors would like to extend their sincere appreciation to Vijaya Sree Dhulipalla, Department of Computer Science and Artificial Intelligence ,KKR and KSR Institute of Technology and Sciences, for their valuable guidance, insightful suggestions, and support through out the course of this project. The authors would like to than KKR and KSR Institute of Technology and Sciences for providing the necessary infrastructure and research facilities that made the successful completion of this work possible.

REFERENCES

[1] S. Liang, Y. Li, and R. Srikant, “Enhancing the reliability of out-of-distribution image detection in neural networks,” 2018.
[2] P.F.FelzenszwalbandD.P.Huttenlocher,“Efficientgraph-basedimagesegmentation,”InternationalJournalofComputerVision,vol.59,no.2, pp.167–181,2004.
[3] J. Pluim and J. M. Fitzpatrick, “Image registration,” IEEE Transaction son Medical Imaging, vol. 22, no. 11, pp. 1341–1343, 2003.
[4] D. W. Townsend and S. R. Cherry, “Combining anatomy and function:Thepathtotrueimagefusion,”EuropeanRadiology,vol.11,no.10, pp.1968–1974,2001.
[5] A. P. James and B. Dasarathy, “Medical image fusion: A survey of the state of the art,” Information Fusion, vol. 19, pp. 4–19, 2014.
[6] M. Larsen, J. Godt, and N. Larsen, “Automated detection of fundusphotographicredlesionsindiabeticretinopathy,”InvestigativeOphthal-mology & Visual Science, vol. 44, no. 2, 2003.
[7] J. C. Boldrick, C. J. Layton, and J. Nguyen, “Evaluation of digital dermoscopy in a pigmented lesion clinic: Clinician versus computer assessment of malignancy risk,” Journal of the American Academy of Dermatology, vol. 56, no. 3, pp. 417–421, 2007.
[8] A.M.AlhadlaqandN.S.Al-Maflehi,“Newmodelforcervicalvertebralbone age estimation in boys,” King Saud University Journal of Dental Sciences, vol. 4, no. 1, pp. 1–5, 2013.
[9] H.A.Ben,H.Yun,andK.Hamid,“A multi scale approach to pixel-level image fusion,” Integrated Computer-Aided Engineering, vol. 12, no. 2, pp.135–146,2005.
[10] R. Singh and A. Khare, “Fusion of multimodal medical images using Daubechies complex wavelet transform: A multiresolution approach, ”Information Fusion, vol. 19, pp. 49–60, 2014.
[11] B. Yang and S. Li, “Pixel-level image fusion with simultaneous orthogonal matching pursuit,” Information Fusion, vol. 13, no. 1, pp. 10–19,2012.
[12] L.Yu,C.Xun,andJ.Cheng,“Amedicalimagefusionmethodbasedonconvolutional neural networks,” in Proc. 20th International Conference on Information Fusion (Fusion), IEEE, 2017.
[13] L.Yu,C.Xun,andR.K.Ward,“Imagefusionwithconvolutionalsparserepresentation,” IEEE Signal Processing Letters, 2016.
[14] X. Hao, G. Zhang, and S. Ma, “Deep learning,” International Journal of Semantic Computing, vol. 10, no. 3, pp. 417–439, 2016.
[15] N. Chabi, M. Yazdi, and M. Entezarmahdi, “An efficient image fusion method based on dual-tree complex wavelet transform,” in Proc. IEEE,2013.
[16] G.PiellaandH.Heijmans,“A new quality metric for image fusion,”in Proc. International Conference on Image Processing (ICIP), IEEE,2003.
[17] Z.WangandQ.Li,“Informationcontentweightingforperceptualimagequality assessment,” IEEE Transactions on Image Processing, vol. 20,no. 5, pp. 1185–1198, 2011.
[18] Y. Liu, S. Liu, and Z. Wang, “A general framework for image fusion based on multi-scale transform and sparse representation,” Information Fusion, vol. 24, pp. 147–164, 2015.
[19] M.Hossny,S.Nahavandi,andD.Creighton,“Commentsoninformationmeasure for performance of image fusion,” Electronics Letters, vol. 44,no. 8, pp. 1066–1067, 2008.

©IJRASET: All Rights are Reserved

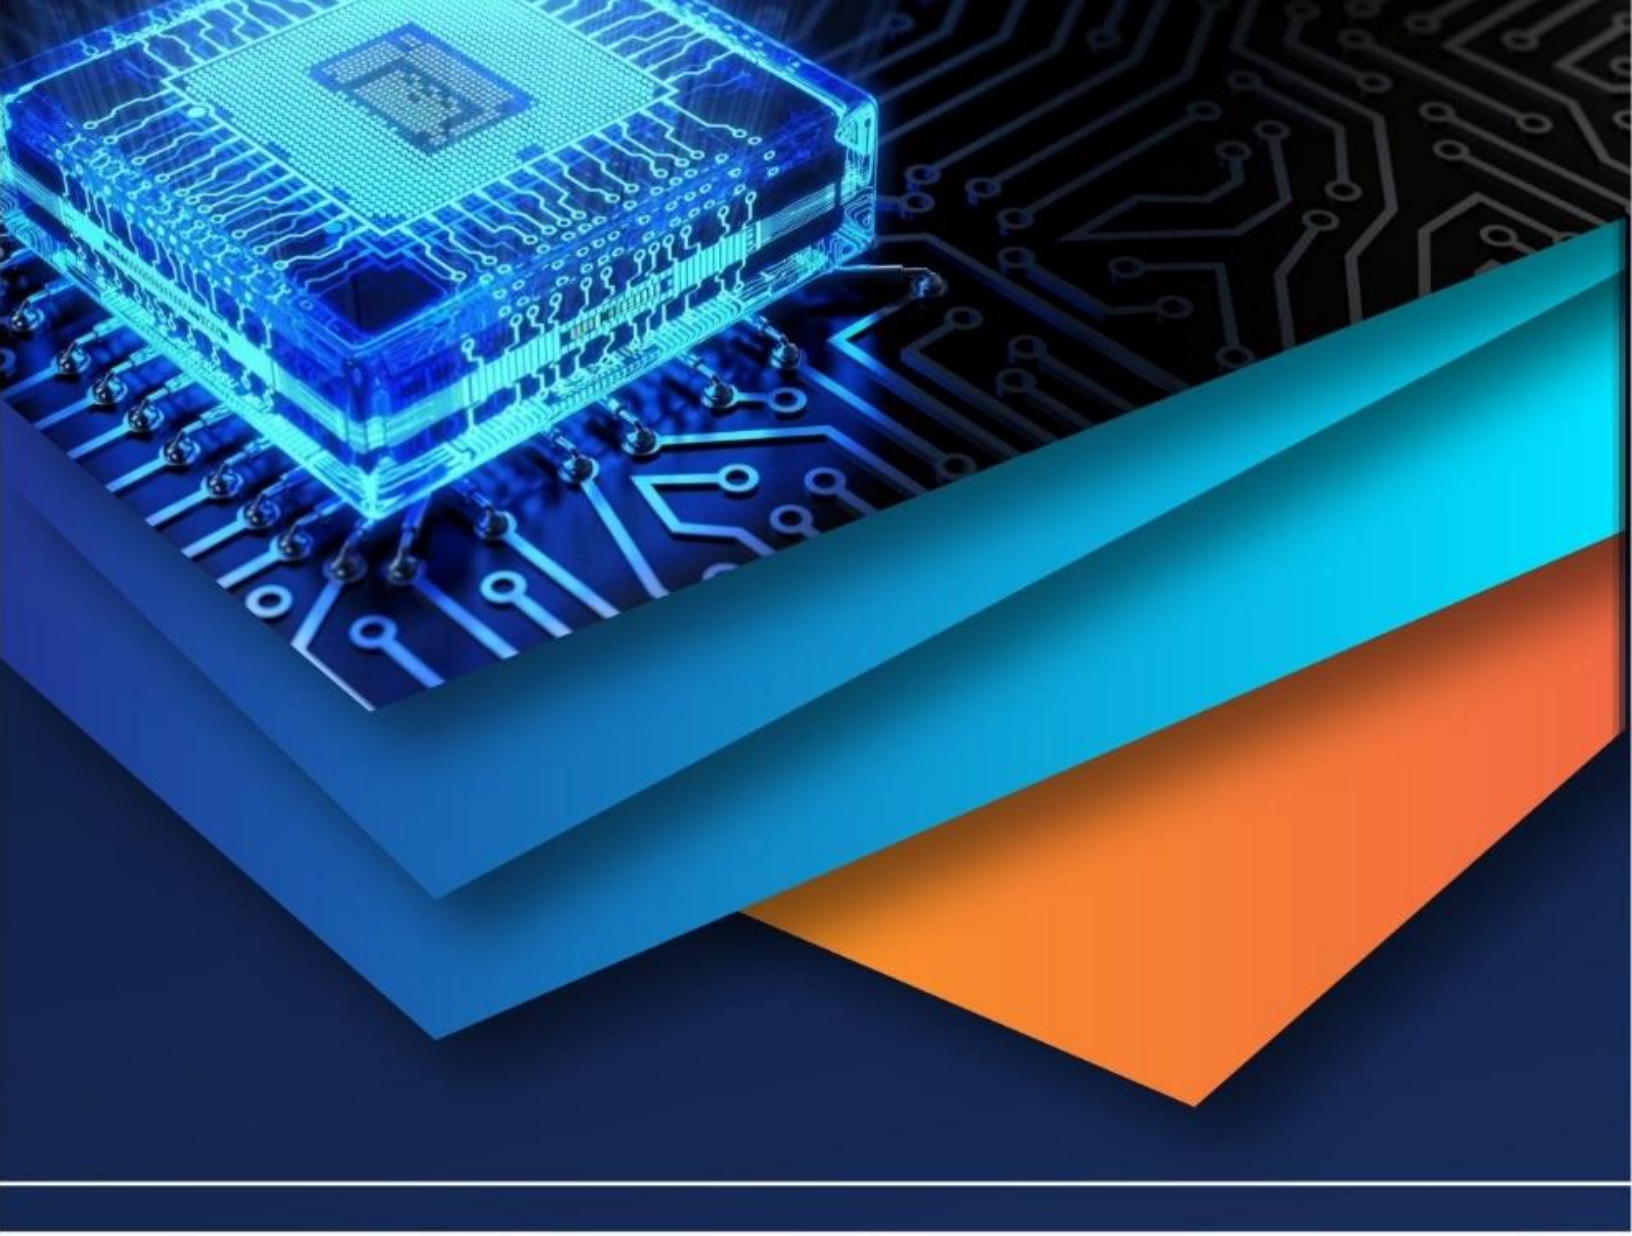

10.22214/IJRASET

45.98

IMPACT FACTOR: 7.129

IMPACT FACTOR: 7.429

INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Call : 08813907089 (24*7 Support on Whatsapp)