iJRASET
International Journal For Research in Applied Science and Engineering Technology



INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Volume: 13 **Issue:** V **Month of publication:** May 2025

DOI: https://doi.org/10.22214/ijraset.2025.71894

www.ijraset.com

Call: 08813907089 | E-mail ID: ijraset@gmail.com

International Journal for Research in Applied Science & Engineering Technology (IJRASET)
ISSN: 2321-9653; IC Value: 45.98; SJ Impact Factor: 7.538
Volume 13 Issue V May 2025- Available at www.ijraset.com

IoT-Based Stress and Non-Invasive Glucose Monitoring System Using Wearable Technology and Edge AI

Mohith D[1], Sneha Patel[2], K. B. Ramesh[3], Haron Khadar[4]
Department of Computer Science and Engineering, RV College of Engineering, Bengaluru, India

Abstract: ***The proposed system is an advanced integration of Internet of Things (IoT) and wearable technology, designed to enable real-time, non-invasive monitoring of both stress levels and blood glucose concentration in humans. It combines physiological sensing, embedded processing, and cloud connectivity to deliver continuous health insights. The stress detection module utilizes a heart rate sensor and a Galvanic Skin Response (GSR) sensor to monitor changes in pulse rate and skin conductivity. For glucose estimation, Near-Infrared (NIR) spectroscopy is employed. An ESP32 microcontroller serves as the system's core, collecting sensor data, preprocessing it, and wirelessly transmitting it to cloud-based dashboards. A Python-based simulation environ- ment facilitates debugging and analysis. The system offers a compact and scalable solution for wearable applications. Future enhancements include machine learning integration for improved calibration and personalization.***
Index Terms: Internet of Things (IoT), Stress Detection, Non- Invasive Glucose Monitoring, Wearable Health Devices, Cyber-Physical Systems, Body Area Networks, Real-Time Monitoring

I. INTRODUCTION

The substantial growth in real-time, continuous health mon- itoring systems has been driven by advancements in wear- able technologies and the increasing demand among health- care professionals for proactive diagnostic tools. Two cru- cial health indicators—psychological stress and blood glucose levels—are of particular importance, as they can lead to hy- pertension, diabetes, and cardiovascular diseases. Traditional stress assessment methods rely on clinical instruments or self- reported measures, often followed by invasive procedures such as finger-prick blood sampling for glucose analysis. These approaches limit the feasibility of frequent and convenient monitoring. By integrating IoT technology with non-invasive sensing techniques, organizations can implement remote and real-time health monitoring in a user-friendly and efficient manner.

II. SYSTEM ARCHITECTURE

The proposed system is designed to non-invasively monitor two critical physiological parameters: stress level and blood glucose concentration. It is built around an ESP32 microcontroller, which serves as the central unit for processing and communication. The architecture integrates biosensors, data processing modules, a cloud platform, and optional components for display and alerts.

A. Hardware Components

- Heart Rate Sensor (MAX30102): Uses photoplethys mography to measure pulse rate.
- Galvanic Skin Response (GSR) Sensor: Measures skin conductance via finger electrodes.
- NIR Sensor (NIR LED + Photodiode): Projects and reflects NIR light to estimate glucose.
- ESP32 Microcontroller: Core processor for sensor input, processing, and Wi-Fi transmission.
- OLED Display: Displays real-time vitals (optional).
- Buzzer: Alerts users during abnormal readings (optional).

B. Software Architecture

- Sensor Acquisition: Analog-to-digital conversion and data reading.
- Processing Layer: Computes stress index and maps NIR to glucose.
- Cloud Communication: Sends data via Wi-Fi to Fire- base or ThingSpeak.

©IJRASET: All Rights are Reserved

III. METHODOLOGY

A. *Sensor Data Acquisition*

The ESP32 collects data from:

- Heart Rate: Peak detection of photoplethysmographic signal.
- GSR: Resistance calculated from voltage divider output.
- NIR: Reflected intensity used for glucose mapping.

B. *Signal Processing and Mapping*

$$\text{Stress Index} = \alpha \cdot \text{HR} + \beta \cdot \frac{}{\text{GSR}} \qquad (1)$$

$$\text{Glucose (mg/dL)} = m \cdot \text{NIR Signal} + c \qquad (2)$$

The proposed system is designed to non-invasively monitor two critical physiological parameters: stress level and blood glucose concentration. It is built around an ESP32 microcon- troller, which serves as the central unit for processing and communication. The architecture integrates biosensors, data

IV. SIMULATION

A. *Simulation Objectives*

To test performance, verify algorithm accuracy, and visualize data.

B. *Environment*

Python 3.x using libraries: numpy, matplotlib, random, and time.

C. *Signal Generation*

- Heart Rate: 65–105 BPM
- GSR: 8–30 kΩ*NIR* : 600 − −2800*units*

D. *Output*

Graphs plotted for HR, GSR, stress index, and glucose levels. Alerts are raised when thresholds are crossed.

E. *Cloud Connectivity*

The ESP32 transmits processed sensor values to Firebase or ThingSpeak using HTTP protocols.

V. RESULT

- Stress Detection: Accurate classification based on HR and GSR.
- Glucose Estimation: Linear mapping produced reliable glucose estimates.
- Cloud Upload: Live values updated to cloud dashboards.

VI. CONCLUSION


The system integrates non-invasive stress and glucose monitoring using IoT. It features wearable design, cloud connectiv- ity, and Python-based simulation for validation. The combined use of MAX30102, GSR, and NIR with ESP32 provides a reliable, scalable health monitoring platform.

REFERENCES

[1] G. Picard, A. Turner, and R. Foster, “Stress detection using wearable physiological and sociometric sensors,” *Computer*, vol. 48, no. 10, pp. 26–33, 2015.
[2] S. A. Inamdar and S. S. Kulkarni, “Stress detection and monitoring using wearable biosensors,” in Proc. IEEE ICCUBEA, 2017.
[3] D. A. Hall and A. T. Bartholomeusz, “Non-invasive glucose sensing using near-infrared spectroscopy,” J. Diabetes Sci. Technol., vol. 5, no. 1, pp. 62–69, 2011.
[4] R. Palaniappan, “Non-invasive monitoring of blood glucose using sen- sors and AI,” Sensors and Materials, vol. 32, no. 7, pp. 2545–2556, 2020.
[5] C. Setz et al., “Discriminating stress from cognitive load using a wearable EDA device,” IEEE Trans. Inf. Technol. Biomed., vol. 14, no. 2, pp. 410–417, 2010.

[6] M. Gjoreski et al., "Continuous stress detection using a wrist device: In laboratory and real life," in Proc. ACM UbiComp, 2016, pp. 1185–1193.
[7] J. A. Healey and R. W. Picard, "Detecting stress during real-world driving tasks using physiological sensors," IEEE Trans. Intell. Transp. Syst., vol. 6, no. 2, pp. 156–166, 2005.
[8] J. Yadav et al., "Prospects and limitations of non-invasive blood glucose monitoring using near-infrared spectroscopy," Biomed. Signal Process. Control, vol. 18, pp. 214–227, 2015.
[9] S. K. Vashist, "Non-invasive glucose monitoring technology in diabetes management: A review," Anal. Chim. Acta, vol. 750, pp. 16–27, 2013.
[10] N. S. Oliver et al., "Glucose sensors: A review of current and emerging technology," Diabet. Med., vol. 26, no. 3, pp. 197–210, 2009.
[11] S. M. R. Islam et al., "The Internet of Things for health care: A comprehensive survey," IEEE Access, vol. 3, pp. 678–708, 2015.
[12] F. Mehmood and M. Ahmad, "A smart IoT-based system for monitoring diabetic patients," Int. J. Adv. Comput. Sci. Appl., vol. 11, no. 6, pp. 1–7, 2020.

©IJRASET: All Rights are Reserved | SJ Impact Factor 7.538 | ISRA Journal Impact Factor 7.894 |

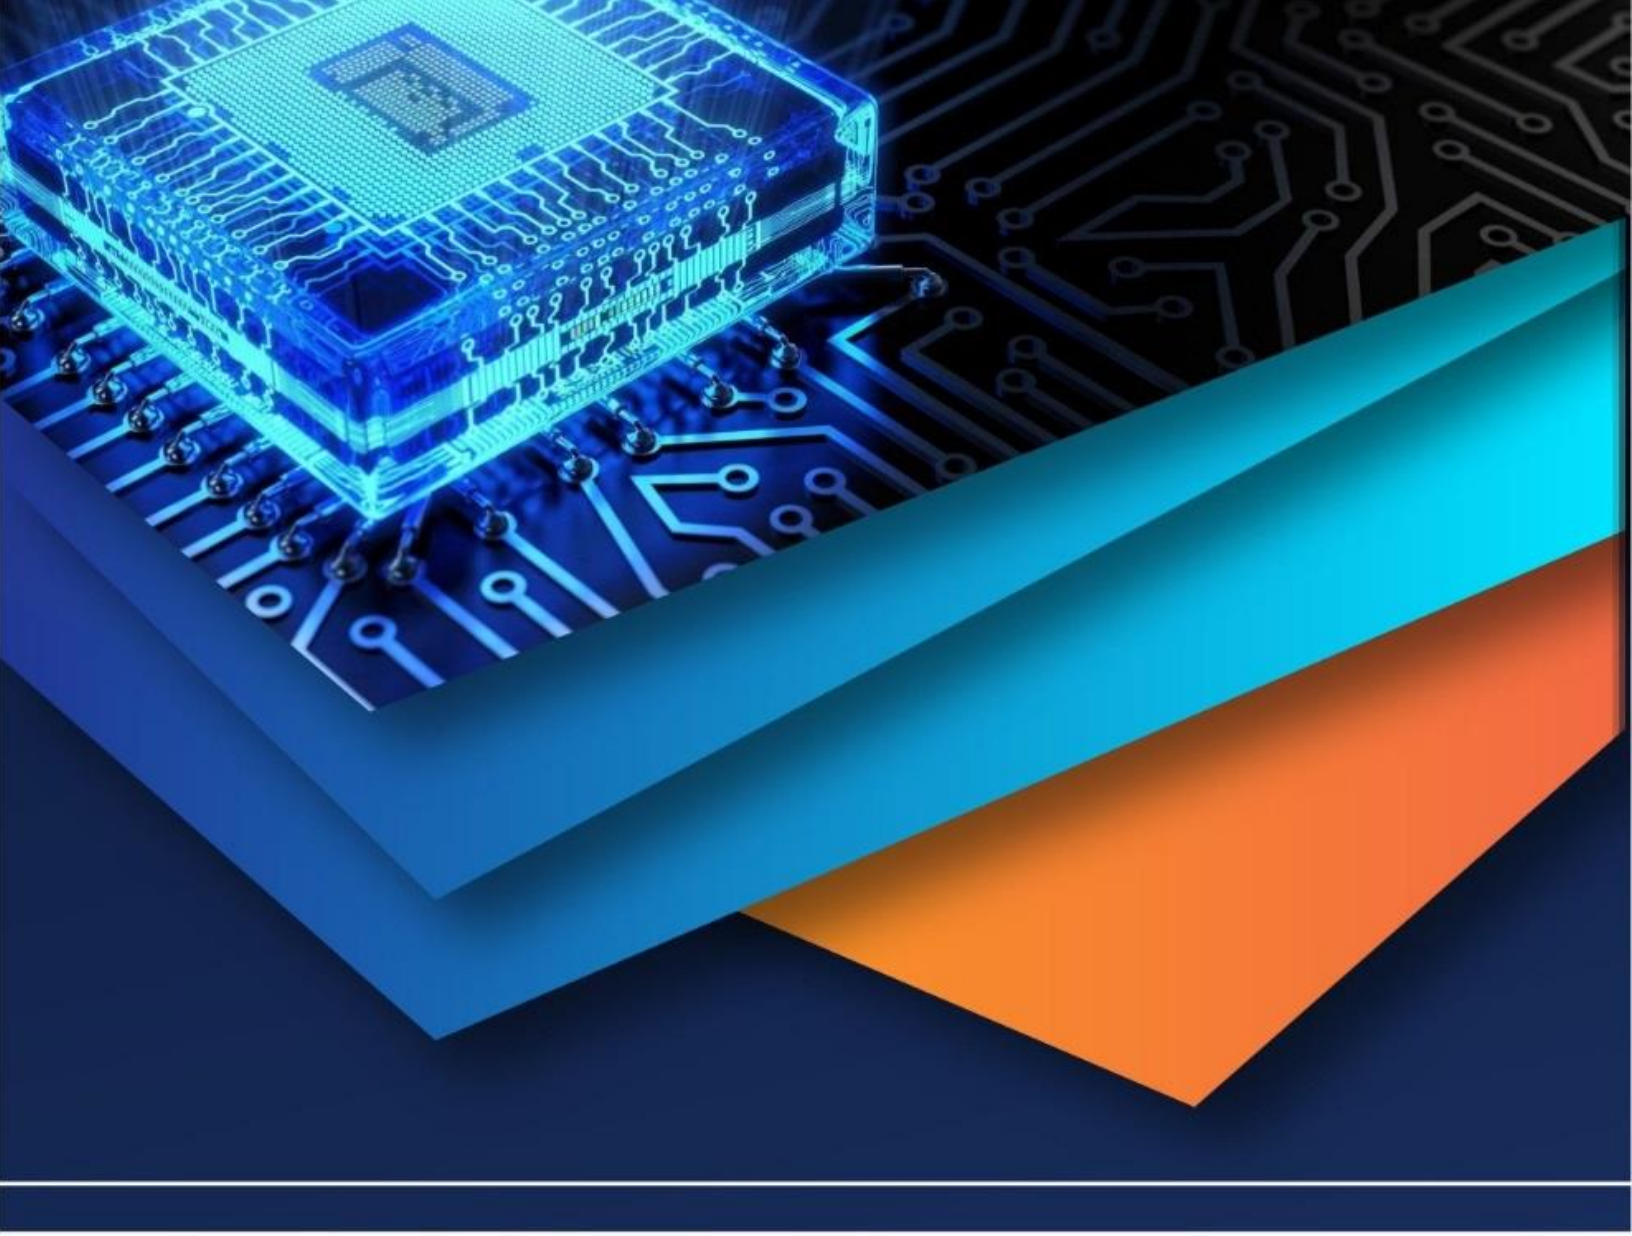

10.22214/IJRASET

45.98

IMPACT FACTOR: 7.129

IMPACT FACTOR: 7.429

INTERNATIONAL JOURNAL FOR RESEARCH

IN APPLIED SCIENCE & ENGINEERING TECHNOLOGY

Call : 08813907089 (24*7 Support on Whatsapp)